



FASTECT 11
IMPORTANT
PLEASE READ!

1. Do not dip the end of the Fastect II past the arrow.
2. Hold the tip of the Fastect II in the urine specimen for 10 seconds, then remove and lay flat.

Dipping the Fastect II past the arrow, or leaving the tip in the urine for longer than 10 seconds, may flood the device and prevent the control line from forming.

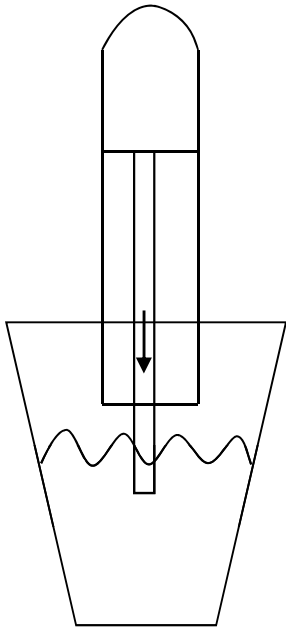

Dip tip into urine for 10 seconds and remove.

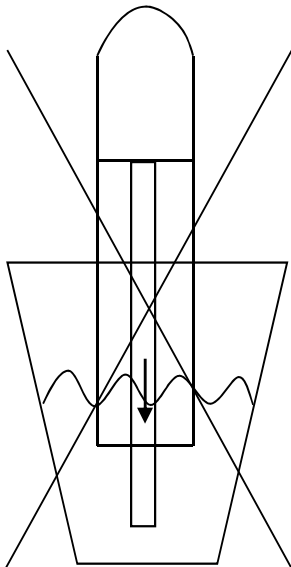

Do not dip plastic or arrow into urine.